

MPT-141-13T

High Field Hall Effect Probe

High Field Application (up to 13 Tesla)

High Accuracy: $\pm 0.05\%$ max. error at 25°C above 2.2T*
Calibration tables at 0, 25 and 50°C supplied

*Contribution of probe



Specifications

The MPT-141-13T High Field Hall Effect Probe is most suitable to be used with a DTM-151 Digital Teslameter. Temperature-compensated from 0 to 50°C up to 2.2 Tesla. Probe can be calibrated to measure field up to 13 Tesla. Transverse orientation reads (+) when field vector enters the top epoxy surface.

Accuracy at 25°C:

$\pm 0.01\%$ of reading + 0.006% of full scale up to 2.2T, temperature-compensated
 $\pm 0.05\%$ of reading + 0.006% of full scale above 2.2T at 25°C

Operating Range:

4- Range Operation
R0.3=1.2, R0.6=2.2, R1.2=2.2, R3.0=13.0 Tesla Full Scale

NOTE: Range R0.3 is calibrated to be read up to 1.2T only. Ranges R0.6 and 1.2 could only display calibrated readings up to 2.2T and are temperature compensated. Reading above 2.2T on those ranges are not calibrated and it is highly recommended to use the top range 13.0 for measurements above 2.2T. This range is only calibrated at 25°C operating temperature.

Temperature Stability:

Calibration: $\pm 10\text{ppm}$ of reading/°C max.
- 3ppm/°C of reading per meter of probe cable
Zero Drift: $\pm (1\mu\text{T} + 0.0003\%$ of full scale)/°C max.

Temperature Range:

0 to 50°C operating to spec, -20 to +60°C max.

ORDER CODE:


MPT-141-13T-7S for probe with basic 5 meters shielded cable.
Special probe cable lengths may be ordered up to 30 meters.

Probe Accessories:

MPT Transverse Probe Holder – Part No. 17000081
MPT Axial Probe Holder – Part No. 17000100

Dimensions:

Probe Head Size: 14 x 5 x 2 mm Sensitive Area: 1 x 0.5 mm
Unshielded part of cable at probe head: 5.0 ± 0.2 mm, 300 mm nominal length
Shielded Cable: $\varnothing 6.5 \pm 0.2$ mm

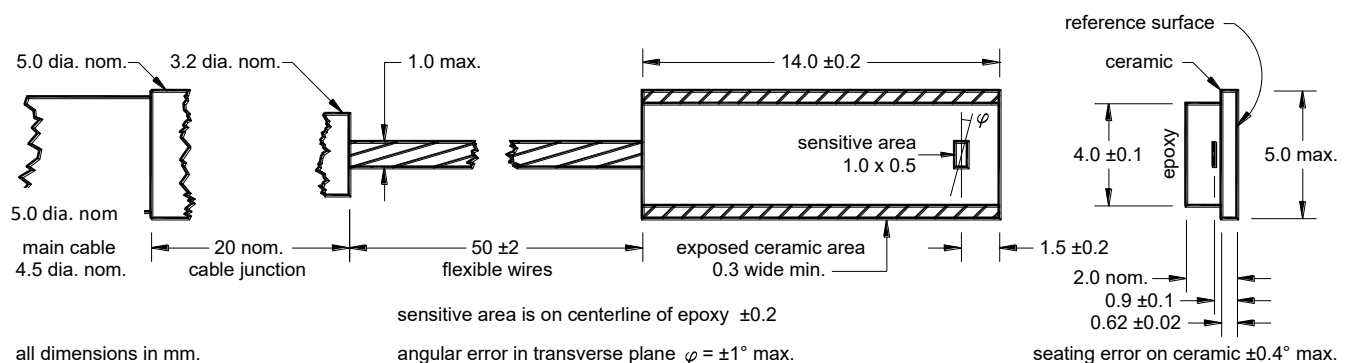

Resolution using DTM-151 Digital Teslameter:

TABLE 1 - DC Mode with Digital Filtering ON
1 in 600,000 bipolar scans in front of panel display

Range	Display resolution		Serial / GPIB Output Resolution	
	Gauss	Tesla	Gauss	Tesla
0.3	0.1	0.00001	0.01	0.000001
0.6	0.01	0.000001	0.01	0.000001
1.2	0.2	0.00002	0.1	0.00001
3.0	1	0.0001	0.1	0.00001

TABLE 2 - DC Mode with Digital Filtering OFF, and AC Mode,
1 in 120,000 bipolar scans in front of panel display

Range	Display resolution		Serial / GPIB Output Resolution	
	Gauss	Tesla	Gauss	Tesla
0.3	0.2	0.00002	0.01	0.000001
0.6	0.5	0.00005	0.01	0.000001
1.2	1	0.0001	0.1	0.00001
3.0	2	0.0002	0.1	0.00001